



ADIAVET™ BoHV-4 REAL TIME

TEST FOR THE DETECTION OF BOVINE HERPESVIRUS TYPE 4 BY REAL-TIME
ENZYMATIC GENE AMPLIFICATION (PCR TEST)

Reference:

ADI481-100 (100 reactions)



NOTE

Dye compounds in this product are sold under license from Biosearch Technologies, Inc. and protected by U.S. and worldwide patents either issued or in application. The license covers Veterinary Molecular Diagnostics.

ADIAVET™ BoHV-4 REAL TIME

I.	REVISION HISTORY	3
II.	GENERAL INFORMATION.....	4
1.	Purpose of the test	4
2.	Pathogen.....	4
3.	Description and purpose of the test	4
III.	MATERIAL AND REAGENTS.....	5
1.	Reagents provided with the kit.....	5
2.	Validity and storage	5
3.	Use of BoHV-4 CTL+	5
4.	Equipment required but not supplied	5
IV.	RECOMMENDATION BEFORE THE ANALYSIS OF SAMPLES	6
1.	Precautions.....	6
2.	Storage of samples and DNA extracts.....	6
3.	Samples preparation	6
4.	Controls to include.....	6
V.	EXTRACTION AND PURIFICATION	8
1.	Using QIAamp® DNA Mini kit	8
2.	Using NucleoSpin® Tissue kit	9
3.	Using DNA/RNA magnetic beads kit	10
VI.	AMPLIFICATION.....	11
VII.	INTERPRETATION OF RESULTS.....	12
1.	Definitions	12
2.	Validation and interpretation of results.....	12
	<i>A. Validation of the run.....</i>	<i>12</i>
	<i>B. Result interpretation.....</i>	<i>13</i>
VIII.	INDEX OF SYMBOLS	14

I. Revision history

N/A	Not Applicable (first publication)
Correction	Correction of document anomalies
Technical change	Addition, revision and/or removal of information related to the product
Administrative	Implementation of non-technical changes noticeable to the user

Note: minor typographical, grammar and formatting changes are not included in the revision history.

Release Date	Part Number	Change type	Change summary
2013/01	NE481-02	Technical change	Addition of "Extraction using DNA/RNA magnetic beads kit" paragraph, in page 10, § V-3.
2014/12	NE481-03	Technical change	Addition of "Index of symbols" section, in page 14.
2014/12	NE481-03	Technical change	Removal of reference ADI481-50 (50 reactions)
2016/07	NE481-04	Administrative	Changing logos
2016/07	NE481-04	Administrative	Biosearch legal mention
2016/07	NE481-04	Administrative	Addition of table "Analysis options according to the specimen" §I.3

II. General information

1. Purpose of the test

ADIAVET™ BoHV-4 REAL TIME kit is intended to detect the Bovine Herpesvirus type 4 (BoHV-4) using real-time Polymerase Chain Reaction (PCR) technology from swab of bovine and from viral culture.

2. Pathogen

BoHV-4 is a DNA virus, member of the subfamily *Gammaherpesvirinae*. It has been isolated the first time in 1966 in Hungary, from calves showing clinical signs of respiratory disease and keratoconjunctivitis (Movar 33/63 strain). Since, virus isolation has been reported in Europe, North America, Africa and Asia from animals showing a variety of clinical signs, such as conjunctivitis, pneumonia, skin lesions, enteritis, ulcerative mammillitis, postpartum and chronic metritis. BoHV-4 can also be isolated from healthy bovine. Therefore, it is sometimes named "passager" virus.

BoHV-4 is mainly isolated from both superior respiratory tract and genital tracks.

The multiplication of virus could take place likely in epithelial cells of mucosa.

The main site of the virus persistence seems to be the monocytes and macrophages in the organism.

The diagnosis can be performed by the detection of the virus by direct methods (viral isolation or PCR) or by indirect immunofluorescence on cell cultures.

3. Description and purpose of the test

This test is based on enzymatic gene amplification or PCR technology.

Amplified products are detected in real-time thanks to a specific labelled hydrolysis probe (5'-exonuclease technology).

The ADIAVET™ BoHV-4 REAL TIME kit enables the simultaneous detection of:

- BoHV-4 target (probe labelled in FAM),
- GAPDH, an internal control of extraction and amplification steps specific from an endogenous DNA (probe labelled with a fluorochrome read in the same spectra as VIC and HEX).

ADIAGENE recommends using this test with DNA purification kits (Qiagen, Macherey-Nagel). Other purification kits can be used if they have been validated by the user.

Analysis options according to the specimen:

Specimen	Individual analysis
Swab (placental, vaginal...)	<input checked="" type="checkbox"/>
Viral culture	<input checked="" type="checkbox"/>

III. Material and reagents

1. Reagents provided with the kit

Designation	Reagent	ADI481-100
A5	Amplification solution	2 x 1000 µl green tubes
BoHV-4 CTL+	Positive control BoHV-4	1 purple tube

2. Validity and storage

On receipt, the kit should be stored at <-15°C.

It is recommended to make fractions of A5 solution if it should be defrosted more than 3 times.

Do not defrost reagents more than 3 times.

Realtime reagents are susceptible to light: store them in the darkness.

The A5 reagent is ready to use for PCR reaction.

Do not mix reagents of two different batches.

3. Use of BoHV-4 CTL+

Add **200 µl** of Nuclease-free water to the BoHV-4 CTL+ tube included in the kit. Homogenize tube contents using a mixer such as vortex, at least 20 seconds. Aliquot this solution by 6 or 12 µl and store them to <-15°C.

For each analysis, we recommend to use 5 µl of BoHV-4 CTL+ in a well.

4. Equipment required but not supplied

Material should be Nuclease-free (e.g. autoclaved 25 minutes twice at +120°C or once 60 minutes at +121°C)

- Thermal cycler with consumables for real-time PCR: 0.2 ml PCR tubes or closed 96-wells PCR plates with optical quality.
- Class II Microbiological Safety Cabinet
- Centrifuge for microtubes, tubes of 5, 10 or 15 ml, 96-wells plate
- Etuve, heating baths or block heaters
- Instrument for homogenous mixing of tubes
- 1 - 10 µl pipette, 20 - 200 µl pipette and 200 - 1000 µl pipette
- Nuclease-free filter tips
- Nuclease-free microtubes: 1.5 ml and 2 ml
- Sterile tube of 5, 10 or 15 ml
- Powder-free gloves
- 96-100% ethanol solution
- PBS 1 X pH 7.4 buffer

- DNA extraction kit (individual columns)

- QIAamp® DNA Mini Kit (Qiagen, 50 tests: ref. 51304 or 250 tests: ref. 51306)
- NucleoSpin® Tissue (Macherey-Nagel, 50 tests: ref.740952.50 or 250 tests: ref. 740952.250)

or

- Automated DNA/RNA extraction kit (magnetic beads)

See the NEKF user manual available on the web site mentioned on the certificate of analysis included in the used ADIAVET™ kit.

IV. Recommendation before the analysis of samples

Before starting the test, read the entire protocol and scrupulously respect it.

1. Precautions

Adiagène has elaborated this PCR test with the use of Qiagen and Macherey-Nagel extraction kits. Other extraction kits can be used with a previous validation.

Follow the supplier's instructions for the storage, the preparation and the use of the extraction reagents.

Some kits include and/or need the use of toxic reagents. These reagents should be used with gloves and into a chemical cabinet.

We strongly recommend that only appropriately trained personnel perform this test. Ensure the accuracy and precision of the micropipettes used. The quality of the obtained results depends upon rigorous respect of good laboratory practices.

The PCR generates large amount of amplified DNA. A few molecules of amplified products are sufficient to generate a positive result. It is important to reserve 2 rooms, one for manipulation of samples to be tested, and another one for amplified products analysis. Do not open the PCR tubes after amplification.

Samples for analysis should be handled and disposed of as biological waste. **Take all measures of security and confinement required for the manipulation of the concerned biological agents.**

We recommend using fractions of demineralised and saline water and to autoclave them 25 minutes at +120°C. Take a new fraction for each new manipulation to avoid contamination.

2. Storage of samples and DNA extracts

Samples can be stored a couple of days at +2/8°C. After 2 days, we recommend to store them at <-15°C. Extracted DNAs are quite sensitive molecules. Crude extracts should be stored at the end of extraction on melting ice or at +2/8°C for 24h hours, then at <-15°C.

3. Samples preparation

See § IV for the extraction and purification of DNA.

4. Controls to include

The use of controls allows verifying the reliability of the results.

The controls are included per trial of analysis. A trial is defined as all the samples treated in the same conditions.

All the steps of the analysis procedure (extraction+amplification), for all the types of samples, are validated with the association of the controls included in the kit.

- The internal endogenous control (GAPDH) naturally found in the samples allows verifying the extraction and amplification steps of each sample.
- The BoHV-4 CTL+ allows validating the amplification of the target.

Other controls must or could be added:

- **Negative control of extraction (required)**

To verify the absence of cross-contamination, at least one negative control must be included per trial. The control is a negative sample, or 200 µl of the buffer used for dilutions (PBS 1X for example).

- **Positive control of extraction (recommended)**

A positive control could be added in each trial. The control is a sample including the BoHV-4 target. It could come from a positive sample available in the laboratory or from a negative sample spiked with a solution of BoHV-4. This positive control will be closed to the limit of detection of the method. It will inform about the fidelity of the obtained results between different trials.

V. Extraction and purification

1. Using QIAamp® DNA Mini kit

All the centrifugations are performed at room temperature.

Before starting the extraction, turn on the heating system at +70°C.

	vaginal or placental swabs	Viral culture
Preparation of the sample	Introduce the swab in a previously identified 2ml-microtube and, if necessary, cut the stem of the sawb. Add 1 ml of PBS buffer 1X pH 7.4 to the swab. Homogenize for 30 seconds. Transfer 200 µl of the supernatant in a previously identified microtube. *	Transfer 200 µl of culture in a previously identified microtube.
Lysis	Add 180 µl of AL buffer , 20 µl of proteinase K . Homogenize. Incubate 10 minutes at +70°C .	
Binding preparation	Add 200 µl of ethanol 100% . Homogenize the mixture by pipeting (~10 times) or by using a mixer such as vortex (~15 seconds).	
Transfer to columns and binding to the membrane	Identify columns, apply the whole obtained solution to the corresponding column. Centrifuge 1 minute at 10 000 g. <i>If the whole sample has not been loaded once, apply the residual volume onto the column and centrifuge 1 minute at 10 000 g.</i>	
1st wash	Change the collection tube and add 500 µl of AW1 buffer to the column. Centrifuge 1 minute at 10 000 g.	
2nd wash	Change the collection tube and add 500 µl of AW2 buffer to the column. Centrifuge 1 minute at 10 000 g.	
Column dry step	Change the collection tube. Centrifuge 3 minutes at 10 000 g.	
Elution	Transfer the column to a microtube. Add 200 µl of AE buffer . Incubate ~1 minute at room temperature and centrifuge 1 minute at 10 000 g.	
Storage	Close the tubes, identify and store at +2/8°C for 24 hours, then at <-15°C.	

* Store the remaining solution at -20°C +/-5°C for an eventual new analysis.

2. Using NucleoSpin® Tissue kit

All the centrifugations are performed at room temperature.

Before starting the extraction, turn on the heating system at +70°C.

	vaginal or placental swabs	Viral culture
Preparation of the sample	<p>Introduce the swab in a previously identified 2ml-microtube and, if necessary, cut the stem of the sawb.</p> <p>Add 1 ml of PBS buffer 1X pH 7.4 to the swab. Homogenize for 30 seconds.</p> <p>Transfer 200 µl of the supernatant in a previously identified microtube. *</p>	<p>Transfer 200 µl of culture in a previously identified microtube.</p>
Lysis	<p>Add 180 µl of B3 buffer and 25 µl of proteinase K. Homogenize.</p> <p>Incubate 10 minutes at +70°C.</p>	
Binding preparation	<p>Add 200 µl of ethanol 100%.</p> <p>Homogenize the mixture by pipeting (~10 times) or by using a mixer such as vortex (~15 seconds).</p>	
Transfer to columns and binding to the membrane	<p>Identify columns, apply the whole obtained solution to the corresponding column.</p> <p>Centrifuge at 10 000 g/1 minute.</p> <p><i>If the whole sample has not been loaded once, apply the residual volume onto the column and centrifuge 1 minute at 10 000 g.</i></p>	
1st wash	<p>Change the collection tube and add 500 µl of BW buffer to the column.</p> <p>Centrifuge 1 minute at 10 000 g.</p>	
2nd wash	<p>Change the collection tube and add 500 µl of B5 buffer to the column.</p> <p>Centrifuge 1 minute at 10 000 g.</p>	
Column dry step	<p>Change the collection tube.</p> <p>Centrifuge 3 minutes at 10 000 g.</p>	
Elution	<p>Transfer the column to a microtube. Add 200 µl of BE buffer.</p> <p>Incubate ~1 minute at room temperature and centrifuge 1 minute at 10 000 g.</p>	
Storage	<p>Close the tubes, identify and store at +2/8°C for 24 hours, then at <-15°C.</p>	

* Store the remaining solution at -20°C +/-5°C for an eventual new analysis.

3. Using DNA/RNA magnetic beads kit

See the NEKF user manual available on the web site mentioned on the certificate of analysis included in the used ADIAVET™ kit

VI. Amplification

a- Determine the number of analysed samples including the controls (e.g. positive and negative extraction controls, positive control of amplification (BoHV-4 CTL+) and No Template Control (NTC)).

b- Defrost the A5 solution at room temperature. Homogenize. Dispense **20 µl** of the A5 solution in each PCR tubes or PCR plate wells with a micropipette with a Nuclease-free tip.

c- **Immediately replace the A5 solution tube at <-15°C and in darkness.**

d- For each sample, the extraction negative control (obligatory) and the extraction positive control (recommended) add **5 µl** of purified extract to the 20 µl of A5 solution.

For the positive control, add **5 µl** of the solution obtained in § II-3 to the 20 µl of A5 solution.

For the No Template Control (NTC), nothing is added to the A5 solution.

Immediately replace purified DNA extracts at +2/8°C or at <-15°C. Take care to have no bubbles in the bottom of the wells.

e- Once all the tubes have been prepared, run the real-time PCR amplification.

The BoHV-4 target is read in FAM. The Internal Control is read in VIC or HEX. The Quencher is non fluorescent. The solution contains a passive reference ROX for the ABI machines. Fluorescence is read during the elongation step (1 minute at 60°C).

The following program is defined for **ABI Prism** thermalcyclers (like 7500, StepOne...) from **Applied Biosystems** (check the "emulation 9600" option if available), for the **Rotorgene** from **Qiagen** and for the **Chromo 4** from **Biorad**:

2 minutes 50°C

10 minutes 95°C

15 seconds at 95°C and 1 minute at 60°C during 45 cycles

This program is concerning the **MX3000P** and **MX3005P** of **Stratagene**:

2 minutes 50°C

10 minutes 95°C

30 seconds at 95°C and 1 minute at 60°C during 45 cycles

Roche diagnostic: LightCycler 2*, LightCycler 480*

*** NOTE:** *The use of LightCycler thermalcyclers requires a calibration manipulation. AdiaGene will furnish process chart and reagents required for this calibration.*

Contact us if you wish to use other thermalcyclers.

VII. Interpretation of results

1. Definitions



The « **base line** » corresponds to the background of fluorescence and qualifies the non-characteristic part of the curve observed during the first cycles.

The « **Characteristic amplification curve** » qualifies a fluorescence curve with an exponential phase, a linear phase and a plateau phase.

The « **threshold line** » has to be placed over the background in the exponential phase of a characteristic amplification curve or a group of characteristic amplification curves.

The « **threshold cycle (Ct)** » of a well corresponds, for each detected fluorophore, at the crossing point of the threshold line with the fluorescent curve. The Ct value expressed by the machine for each well depends on the threshold position and on the quantity of target sequences initially present in the PCR well.

Example of characteristic amplification curve

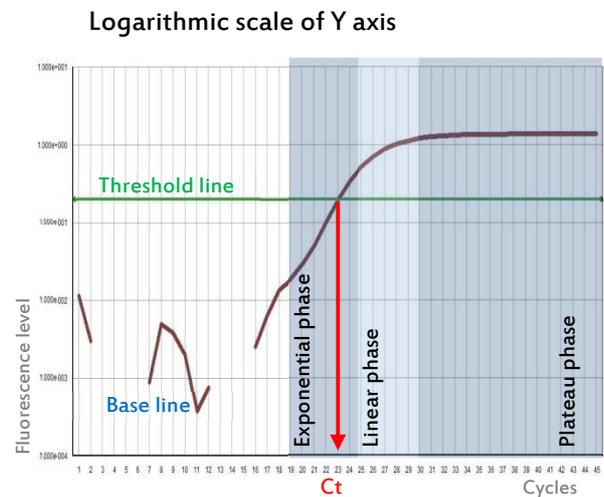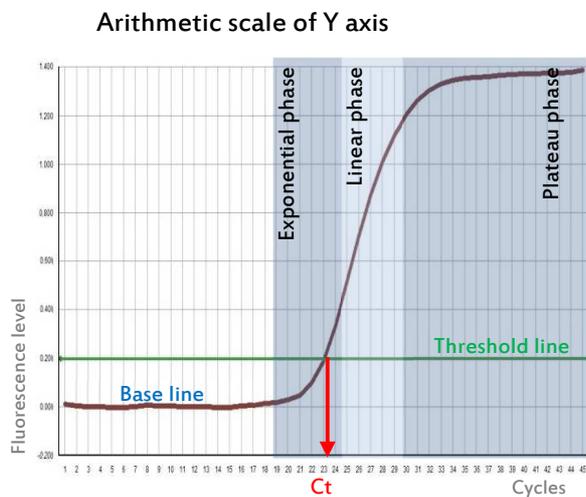

2. Validation and interpretation of results

Display the FAM curves from the plate and set the threshold value as indicated above.

Proceed in the same mean for the VIC or HEX curves.

A. Validation of the run

Amplification is considered to be **valid** if the following results are obtained for the controls:

Controls	No Template Control (NTC)	BoHV-4 CTL+	Extraction negative control	Extraction positive control *
FAM amplification	no	yes	no	yes
VIC/HEX amplification	no	no/yes	no	no/yes
Validation of	Absence of contamination for amplification	Amplification of the target	Absence of contamination for extraction	Extraction and amplification steps

* Optional

The indicative Ct values (FAM and VIC/HEX dyes) of the positive control are indicated in the certificate of analysis of the kit.

B. Result interpretation

DNA extraction and amplification for each sample are considered to be **valid** if at least a characteristic amplification curve is observed for BoHV-4 (FAM) and/or for the internal control (VIC or HEX).

Example	A	B	C	D
FAM amplification	no	yes	yes	no
VIC/HEX amplification	yes	no	yes	no
Result	negative	positive	positive	undetermined

The sample is considered as **negative** if a characteristic amplification curve is observed in VIC or HEX without any amplification in FAM (example A).

The sample is considered as **positive** if a characteristic amplification curve is observed in FAM (example B). Internal control can be co-amplified (example C).

A total absence of characteristic amplification curve for a sample (example D) shows a defective DNA extraction (lost or destruction of DNA) or a deficient real-time PCR (inhibitors in the sample, program error or no template added). In this case, we recommend first to repeat the test with pure and tenfold diluted DNA in Nuclease-free water. Then, if the test is still not valid, a new extraction is recommended.

VIII. Index of symbols

Symbol	Meaning
	Catalogue number
	Manufacturer
	Upper temperature limit
	Use by date
	Batch code
	Consult Instructions for Use
	Contains sufficient for <n> tests
	Keep away from sunlight
	For veterinary in vitro use only – For animal use only

Bio-X Diagnostics, the logos, ADIAGENE and ADIAVET™ are used, pending and/or registered trademarks belonging to ADIAGENE and/or Bio-X Diagnostics, or one of its subsidiaries, or one of its companies. Any other name or trademark is the property of its respective owner.



**S.A.R.L. ADIAGENE**
9, rue Gabriel Calloët-Kerbrat
22440 Ploufragan - France

RCS 417 876 299
Tel. +33 (0)2 96 68 40 20
www.biox.com